



70u 3B 5G 3R 7V

Cytometer:	FACSriaIII	User:	Administrator
Cytometer Name:	FACSriaIII	Institution:	N/A
Serial Number:	P99900016	Software:	BD FACSDiva 8.0
Input Device:	Manual	Date:	2/7/2017 3:51:02 PM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	2.00		


Blue Laser
(488nm)
FSC

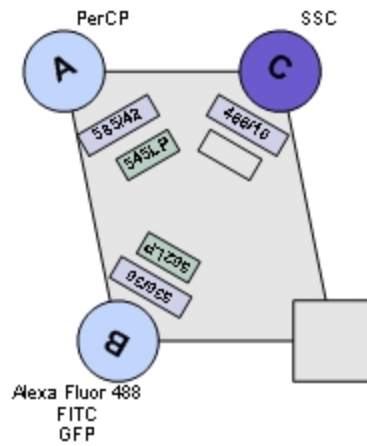


561 Yellow-Green Laser
(561nm)

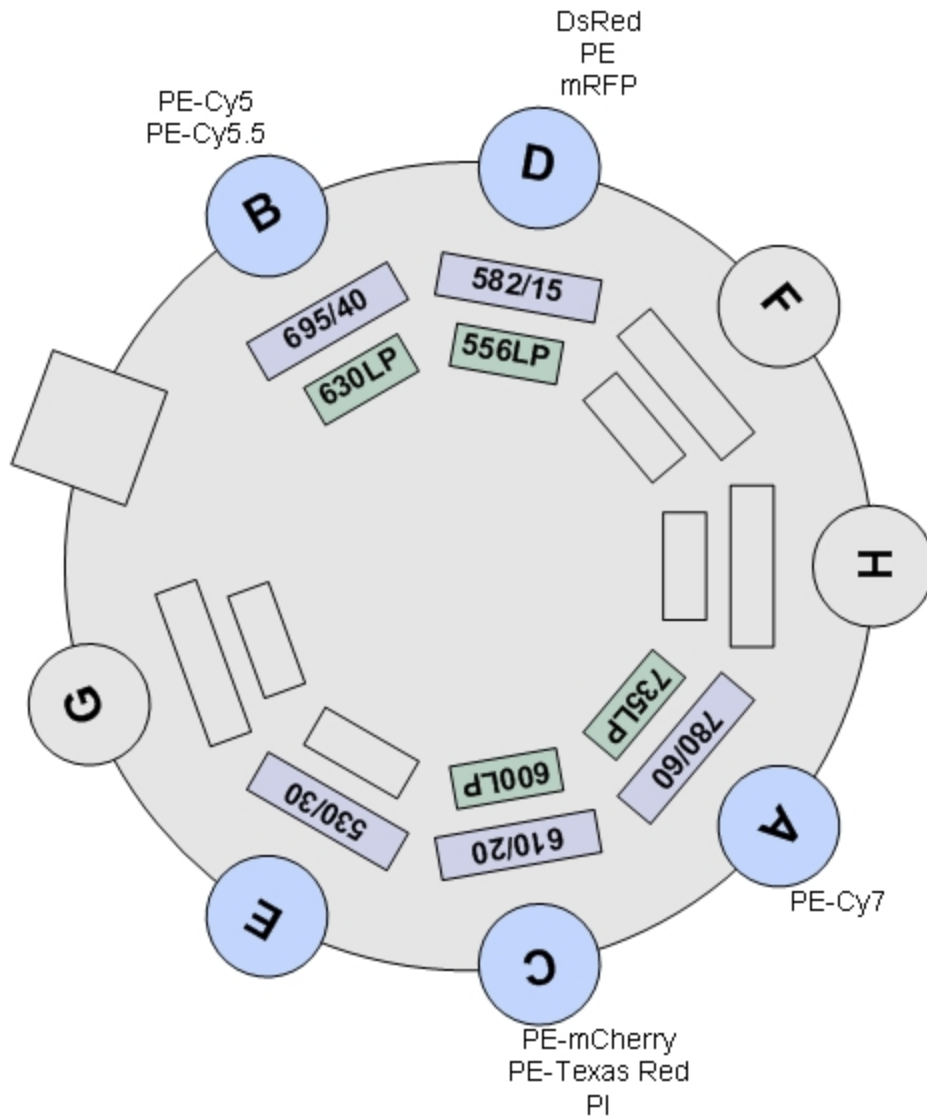

Red Laser
(633nm)

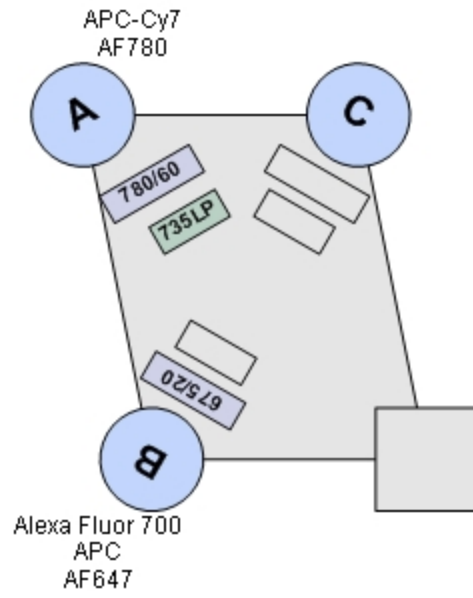

Violet Laser
(407nm)

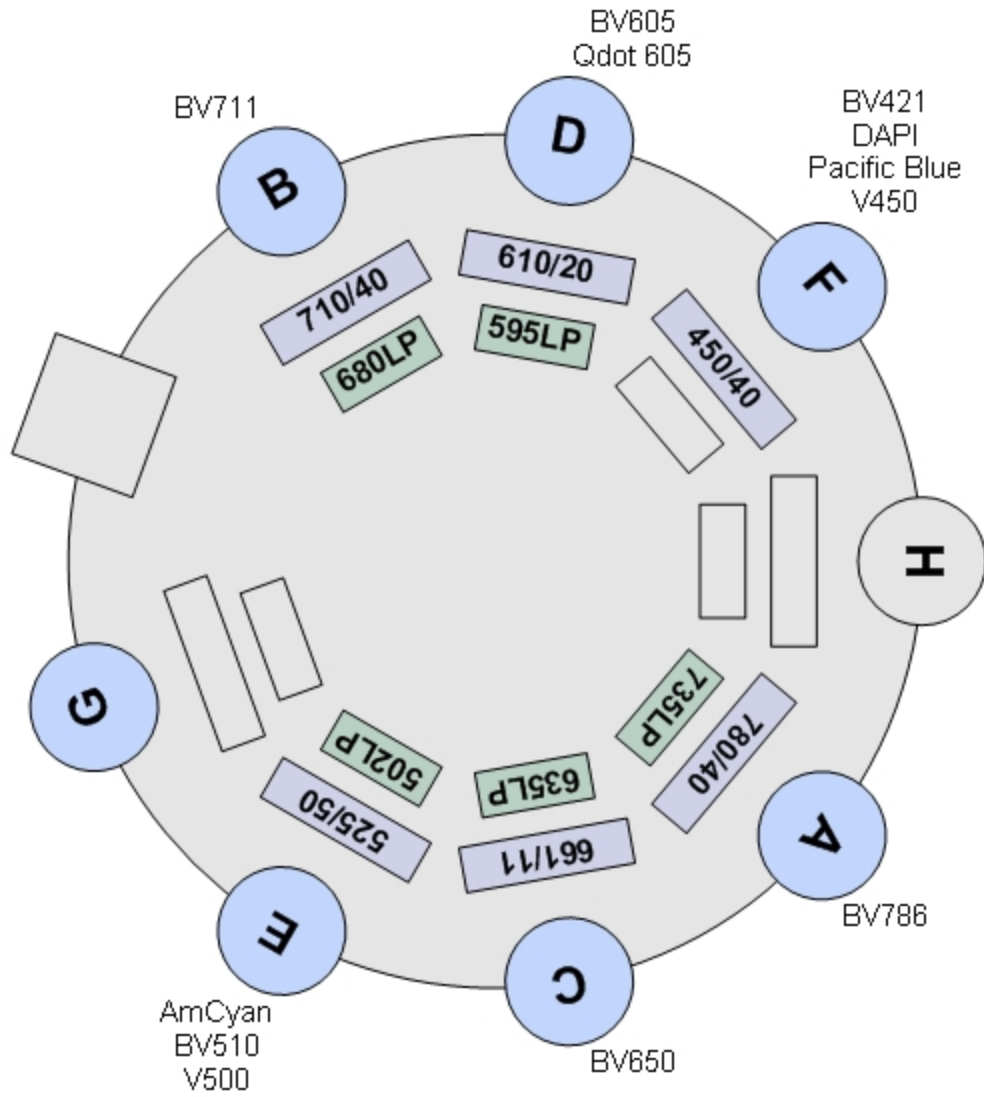

Comments: